

Ratio of Axial Length to Corneal Radius in Japanese Patients and Accuracy of Intraocular Lens Power Calculation Based on Biometric Data



MIKI KAMIKAWATOKO OMOTO, HIDEMASA TORII, KEN HAYASHI, MASAHIKO AYAKI, KAZUO TSUBOTA, AND KAZUNO NEGISHI

- **PURPOSE:** To evaluate the features of the axial length-to-corneal radius (AL/CR) ratio in Japanese patients with cataracts and to determine the accuracy of intraocular lens (IOL) power calculation formulas according to the AL/CR features and the axial length (AL).

- **DESIGN:** Retrospective observational case series.

- **METHODS:** Setting was a clinical practice. Patient population was a total of 1,135 eyes (1,135 patients) with cataracts. Observation procedures included measurement of the AL and corneal radius (CR) by optical biometry and evaluation of the refractive outcomes by using the SRK/T, Holladay 1, Hoffer Q, Haigis, and Barrett Universal II formulas. Main outcome measurements were the features of the AL/CR ratio and the accuracy of IOL power calculations based on the AL/CR ratio and the AL.

- **RESULTS:** The mean AL/CR ratio was 3.15 ± 0.19 . Significant weak negative correlations were observed between the spherical equivalent (SE) and AL ($r = -0.7489$; $P < .001$) and between the SE and AL/CR ratio ($r = -0.8069$; $P < .001$); no correlation was found between the SE and CR ($r = 0.0208$, $P = .483$). For medium ALs and high AL/CR ratios, the SRK/T formula performed less accurately. For long ALs and high AL/CR ratios, the Holladay 1 and Hoffer Q formulas performed less accurately. The Barrett Universal II formula performed well across a range of ALs and AL/CR ratios.

- **CONCLUSIONS:** The AL/CR ratio explained the total variation in the SE better than the AL alone. Surgeons should pay attention to the selection of IOL power calculation formulas in eyes with high AL/CR ratios. (Am J Ophthalmol 2020;218:320–329. © 2020 The Authors. Published by Elsevier Inc. This is an open access article

under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

CATARACT SURGERIES ARE BOTH REHABILITATIVE and refractive procedures. With modern surgical techniques, patients' expectations for perfect postoperative vision are increasing day by day. Partial coherence interferometry has increased the precision of the preoperative measurements, leading to improved postoperative refractive results.^{1,2} Postoperative refractive errors depend mainly on 4 factors: corneal power, axial length (AL), intraocular lens (IOL) type, and postoperative anterior chamber depth (ACD).^{3–5} Popular third-generation formulas (ie, the Hoffer Q,⁶ the SRK/T,⁷ and the Holladay 1)⁸ calculate the theoretical effective lens position (ELP) using the AL and corneal power. The newer fourth- and fifth-generation formulas, Haigis¹ and Barrett Universal II,⁹ respectively, include additional parameters for calculating the ELP, including the preoperative ACD in the Haigis formula and lens thickness; ACD; and the corneal white-to-white value in the Barrett Universal II.

Modern IOL calculation formulas show similarly accurate refractive outcomes in eyes with normal ALs.^{10–12} However, among the wide range of available IOL power formulas, none is completely accurate in all scenarios. Considering that each formula determines the ELP in different ways based on the input variables, certain formulas should be more accurate under specific conditions related to the input variables used, such as the AL and corneal keratometry reading. Recently, 3 new methods of IOL power selection, the Ladas Super Formula,¹³ the FullMonte IOL method,¹⁴ and the Hill-Radial Basis Function method,¹⁵ have been proposed. These methods predict the refractive outcomes by considering the particular combination of AL and keratometry or by pattern recognition. However, the prediction errors using these new methods have not surpassed those of the conventional methods.¹⁶

Refractive errors, which are related closely to visual function, vary among populations.^{17–23} In addition, the optimized lens constants for IOL calculation differ according to race.²⁴ Therefore, the refractive outcomes of

Accepted for publication Mar 6, 2020.

From the Department of Ophthalmology (M.K.O., H.T., K.H., K.T., K.N.), Keio University School of Medicine, Tokyo, Japan; Hayashi Eye Hospital (K.H.), Fukuoka, Japan; and Otake Clinic Moon View Eye Center (M.A.), Kanagawa, Japan.

Inquiries to Kazuno Negishi, Department of Ophthalmology, Keio University School of Medicine, 35 Shinanomachi, Shinjuku-ku, Tokyo 1608582, Japan; e-mail: kazunonegishi@keio.jp

cataract surgeries in previous reports from Western countries may not be applicable to Asian eyes.

Grosvenor²⁵ first reported an association between the AL and the axial length-to-corneal radius (AL/CR) ratio and the refractive status. The AL/CR ratio then was found to be related more closely to refraction than the AL or CR alone.^{26–32} He and colleagues²⁶ reported that the AL/CR ratio generally can determine the refractive status of the human eye and described the shape of the globe. Therefore, this study hypothesized that the AL and the AL/CR ratio may play important roles in the inaccuracy of the IOL power calculations.

The first aim of the current study was to evaluate the AL/CR ratio features of patients with cataracts in Japan and the relationship between the preoperative spherical equivalent (SE) refraction and the preoperative measurements of the AL, CR, and AL/CR ratio. The second aim was to investigate the accuracy of the IOL power calculations according to the AL/CR ratio features and the AL by using 5 IOL power calculation formulas (ie, the SRK/T, the Holladay 1, the Hoffer Q, the Haigis, and the Barrett Universal II formulas).

METHODS

A RETROSPECTIVE CHART REVIEW WAS PERFORMED OF PATIENTS who underwent uneventful sutureless phacoemulsification cataract surgery with in-the-bag implantation of an AcrySof IQ SN60WF IOL (Alcon Laboratories, Inc., Fort Worth, Texas) through a limbal or clear corneal incision of 2.0- to 2.4-mm at the Hayashi Eye Hospital. Seven surgeons (K.H., K.Y., K.H., T.Y., S.M., T.S., and H.S.) performed all surgeries between February 2017 and January 2019. All patients underwent preoperative biometric measurements using a swept-source optical coherence tomography device (IOLMaster 700, Carl Zeiss Meditec, Jena, Germany). If patients underwent bilateral surgeries, the study eye was selected randomly. The exclusion criteria were eyes with a history of previous corneal or intraocular surgeries, any corneal disease, and a postoperative best-corrected visual acuity less than 0.8 (20/25) for any reason. In addition, 2 patients with AL exceeding 30 mm (ALs of 30.08 and 31.6 mm) also were excluded because of the extremely small number of cases. All patients provided written informed consent before the surgeries, and opt-out consent was used to participate in this study. The Institutional Review Board of Hayashi Eye Hospital, Fukuoka, Japan, approved this study.

Preoperatively, the IOL powers were calculated using the SRK/T, Holladay 1, Hoffer Q, Haigis, and Barrett Universal II formulas. Data were collected from the partial coherence interferometry device and from the electronic medical records. Subjective refraction was performed in all patients 2 months after surgery. The prediction error then was

calculated as the actual postoperative SE minus the refractive result predicted by each formula. Thus, a positive prediction error indicated a refractive outcome that was more hyperopic than predicted. The IOL constants for the Zeiss IOLMaster from the User Group for Laser Interference Biometry online tables³³ were used (IOL constant A of 119.0 for the SRK/T formula; surgeon factor 1.84 for the Holladay 1 formula; personalized ACD of 5.64 for the Hoffer Q formula; a0 of -0.769 and a1 of 0.234 and a2 of 0.217 for the Haigis formula; and lens factor 1.88 for the Barrett Universal II formula).

The mean prediction error (ME), the median absolute prediction error (MedAE), and the mean absolute prediction error were calculated for each formula. The percentages of eyes with a prediction error of ± 0.50 diopter (D) were calculated for each formula. The eyes were divided into 9 subgroups according to the AL (short, <22.0 mm; medium, ≥ 22.0 - <26.0 mm; long, ≥ 26.0 mm) and the AL/CR ratio depending on the 10th and 90th percentiles (<2.95 , ≥ 2.95 , and <3.43 , ≥ 3.43 , respectively).

Statistical analyses were performed using the SPSS version 22 software (IBM, Armonk, New York) for Microsoft (Redmond, Washington) and JMP Pro version 19 (SAS Institute, Cary, North Carolina). Because the AL and AL/CR ratio were not distributed normally, the Mann-Whitney *U* test was used to compare the unpaired samples. The associations among the SE and AL, CR, or AL/CR ratio were examined using correlation analyses, and the Z-test was used to compare distributions. The Friedman test with a Bonferroni correction was used to compare the prediction errors with the 5 IOL power calculation formulas in each subgroup. The percentages of eyes within the ± 0.50 D limit of the target refraction among the formulas were assessed using the Cochran Q test with a Bonferroni correction. The Bonferroni correction was used for multiple comparisons. Statistical significance was set at a *P* value $< .05$.

RESULTS

THE STUDY SAMPLE CONSISTED OF 1,135 EYES (568 RIGHT eyes) of 1,135 patients (684 women). The mean patient age at the time of surgery was 73.1 ± 7.8 years old (range, 43-93 years old). The mean AL was 24.00 mm (range, 21.12-29.73 mm). The mean CR was 7.63 mm (range, 6.79-8.40 mm).

• **AL/CR RATIO AND RELATIONSHIPS AMONG SE AND AL, CR, AND AL/CR RATIO:** The AL/CR ratio exhibited a non-normal distribution (median, 3.10; range, 2.74-3.91). For men and women, respectively, the mean ALs were 24.51 ± 1.50 and 23.65 ± 1.45 mm; the mean CRs were 7.70 ± 0.24 and 7.58 ± 0.25 ; and the mean AL/CR ratios

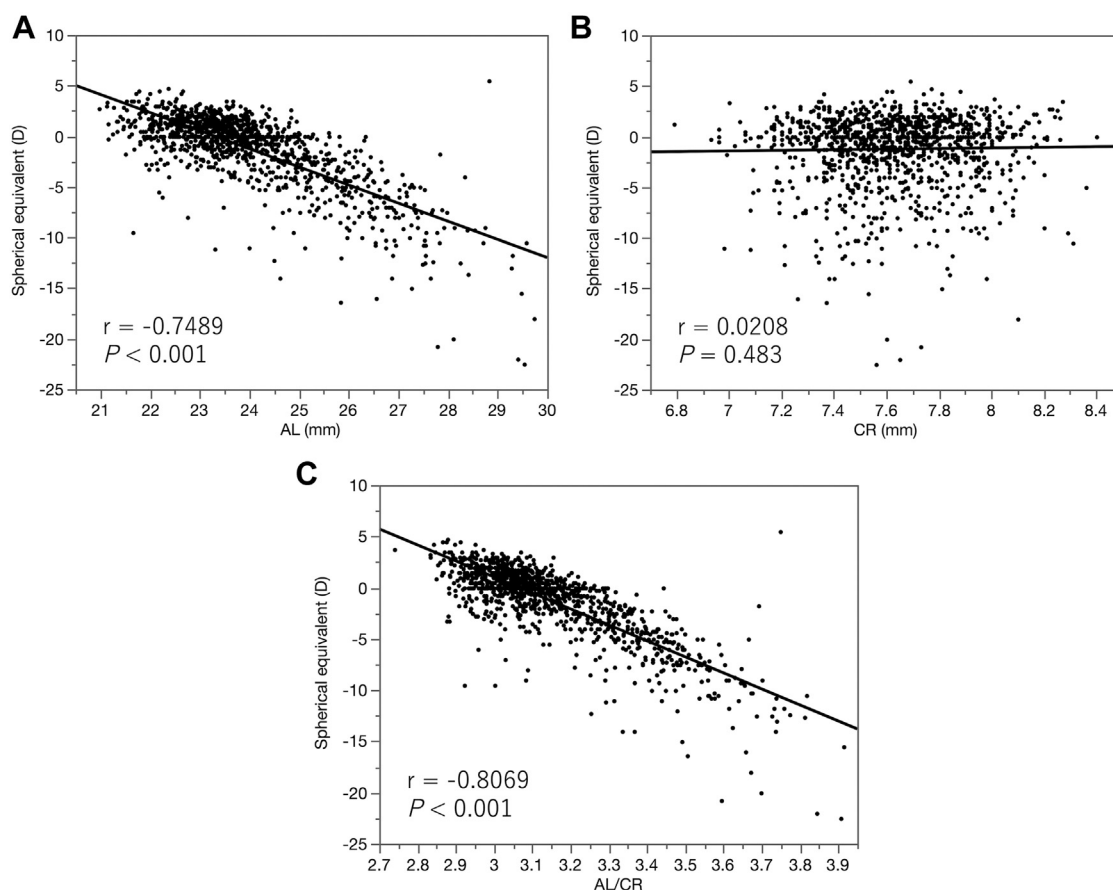


FIGURE 1. A: Scatterplots of AL and spherical equivalent; B: Scatterplots of CR and spherical equivalent; C: Scatterplots of AL/CR and spherical equivalent; AL = axial length; AL/CR ratio = axial length-to-corneal radius ratio; CR = corneal radius; D = diopters.

were 3.18 ± 0.19 and 3.12 ± 0.18 . All differences reached significance ($P < .05$ for all comparisons).

Distributions of the SE and AL, CR, and AL/CR ratio are shown in Figure 1. Significantly weak negative relationships were observed between the SE and AL ($r = -0.7489$; $P < .001$) and between the SE and AL/CR ratio ($r = -0.8069$; $P < .001$), both of which reached significance ($P < .001$). No correlation was found between the SE and CR ($r = 0.0208$; $P = .483$).

• **ACCURACY OF IOL POWER CALCULATIONS ACCORDING TO THE AL AND AL/CR RATIO:** For analytical purposes, the patients were divided into 9 groups according to the AL and AL/CR ratio (Table 1). Figure 2 shows the distributions of the numerical prediction errors in each subgroup. In groups 1 and 4, the Hoffer Q formula had significantly ($P < .05$) negative numerical errors compared with the other 4 formulas (MEs, -0.24 D and -0.19 D, respectively, in groups 1 and 4). In group 2, the Hoffer Q formula also had a significantly ($P < .05$) negative numerical error (ME, -0.20 D) compared with the Holladay 1, Haigis, and Barrett Universal II formulas, whereas the Haigis formula had a significantly ($P < .05$) positive numerical error

(ME, 0.20 D) compared with the other 4 formulas. In group 6, the SRK/T formula had a significantly ($P < .001$) negative numerical error (ME, -0.49 D) compared with the Hoffer Q, Haigis, and Barrett Universal II formulas. The Hoffer Q formula had a significantly ($P < .001$) positive numerical error (ME, 0.33 D) compared with the SRK/T, Holladay 1, and Barrett Universal II formulas. In group 8, the Holladay 1 formula had a significantly ($P < .001$) positive numerical error (ME, 0.28 D) compared with the other 4 formulas. In group 9, the Holladay 1 and Hoffer Q formulas had significantly ($P < .001$) positive numerical errors compared with the other 3 formulas (MEs, -0.43 D and 0.43 D, respectively).

Table 2 shows the MedAEs and mean absolute prediction errors of each formula plotted according to the AL and AL/CR ratio subgroups. In groups 1, 2, 4, 5, and 8, no significant differences were seen among the formulas. In group 6, the MedAE of the SRK/T formula was significantly ($P < .05$) larger than those of the Holladay 1 and Barrett Universal II formulas. The MedAE of the Hoffer Q formula was significantly ($P < .05$) larger than those of the Holladay 1 formula. In group 9, the MedAE of the Holladay 1 formula was significantly ($P < .05$) larger

TABLE 1. Nine Subgroups According to the AL and AL/CR (10th and 90th Percentiles)

	Low AL/CR (AL/CR <2.95)	Moderate AL/CR (2.95 ≤AL/CR <3.43)	High AL/CR (3.43 ≤ AL/CR)
Short AL (AL < 22.0 mm)	Group 1 (n = 29; 2.5%)	Group 2 (n = 33; 2.9%)	Group 3 (n = 0)
Medium AL (22.0 ≤ AL < 26.0 mm)	Group 4 (n = 84; 7.4%)	Group 5 (n = 832; 73.3%)	Group 6 (n = 26; 2.3%)
Long AL (26.0 mm ≤ AL < 30.0 mm)	Group 7 (n = 0)	Group 8 (n = 44; 3.9%)	Group 9 (n = 87; 7.7%)

AL = axial length; AL/CR = axial length to corneal radius ratio; CR = corneal radius.

than those of the SRK/T, Haigis, and Barrett Universal II formulas, and the MedAE of the Hoffer Q formula was significantly ($P < .05$) larger than those of the SRK/T, Haigis, and Barrett Universal II formulas.

The percentages of eyes within the ± 0.50 -D and ± 1.00 -D errors are shown in Table 3. For eyes with a short AL (groups 1 and 2), no significant differences were seen. In groups 4 and 5, no significant differences were seen, whereas in group 6, the SRK/T formula produced a significantly ($P < .05$) smaller percentage of eyes within a ± 0.50 -D error than the Barrett Universal II formula. In group 8, the Holladay 1 formula produced a significantly ($P < .05$) smaller percentage of eyes within a ± 0.50 -D error than the Haigis and Barrett Universal II formulas. In group 9, the Holladay 1 formula produced a significantly ($P < .05$) smaller percentage of eyes within a ± 0.50 -D error than the Haigis and Barrett Universal II formulas. Further, the Hoffer Q formula produced a significantly ($P < .05$) smaller percentage of eyes within a ± 0.50 -D error than the SRK/T, Haigis, and Barrett Universal II formulas.

DISCUSSION

TO THE BEST OF THE AUTHORS' KNOWLEDGE, THIS IS THE first study of the AL/CR ratio and the accuracy of IOL power calculations based on the AL and AL/CR ratio using one IOL model in Japan.

• **AL/CR RATIO AND RELATIONSHIPS AMONG THE SE AND AL, CR, AND AL/CR RATIO:** The distributions of the AL/CR ratio have been reported in different populations and age groups^{31,34-41} and the AL/CR ratios for myopia were between 2.9 and 3.1 and less than 2.9 for emmetropia and hyperopia.^{26,27,42-46} Table 4 summarizes the other studies. In the current report, the CR was approximately the same as that in those previous reports, and women had significantly steeper corneal curvature values,⁴³ whereas the current AL was longer than those reported previously. Therefore, the mean AL/CR ratio became the highest. This difference may be due to the higher prevalence of myopia in Japan.^{22,23} Myopia is one of the most common ocular disorders in schoolchildren, and the prevalence of myopia has been reported to be high in East

Asia.^{47,48} In the future, because this tendency may intensify, it is important to improve the accuracy of refractive calculations in eyes with a high AL/CR ratio.

In the current study, the correlation coefficient of the AL/CR ratio with the SE was greater than that of the AL with the SE; therefore, the AL/CR ratio may explain the total variation in the SE better than the AL alone. This trend also has been reported previously,^{26,38} and the current results agreed with them.

• **ACCURACY OF IOL POWER CALCULATIONS ACCORDING TO AL AND AL/CR RATIO:** Previous studies have reported that the Barrett Universal II formula provided better results than the SRK/T, Haigis, Hoffer Q, and Holladay 1 formulas.^{12,29,30} The current results showed that the Barrett Universal II formulas performed well across a range of ALs and AL/CR ratios. The third-generation formulas, including the SRK/T, Hoffer Q, and Holladay 1, were less accurate than the Haigis and Barrett Universal II formulas in eyes with medium and long ALs with high AL/CR ratios. In eyes with low and medium AL/CR ratios, the third-generation formulas were similarly as accurate as the Haigis and Barrett Universal II formulas regardless of the ALs.

Norrby⁴ reported that the preoperative estimation of the postoperative IOL position, postoperative refraction determination, and preoperative AL measurement were the largest contributors of error.

The refractive outcomes for hyperopic patients with short ALs are less accurate, with prediction errors increasing with increasing hyperopia.⁴⁹ This occurs because of difficulties in calculating the true ELP position, because the anterior segment in short eyes is not proportional to the AL.⁵⁰ Because higher IOL powers are needed for emmetropia as a result of the shorter ALs, any inaccuracy in the ELP has an exaggerated effect. Consistent with previous studies,^{12,51,52} the current results did not identify significant differences among the formulas, including the Barrett Universal II formula in short eyes. Moreover, previous studies have reported that the Hoffer Q formula produced slightly myopic refractive errors.^{12,51,52} Shrivastava and colleagues⁵² reported that the Haigis formula produced slightly hyperopic refractive errors. The current findings agreed well with those reported previously.

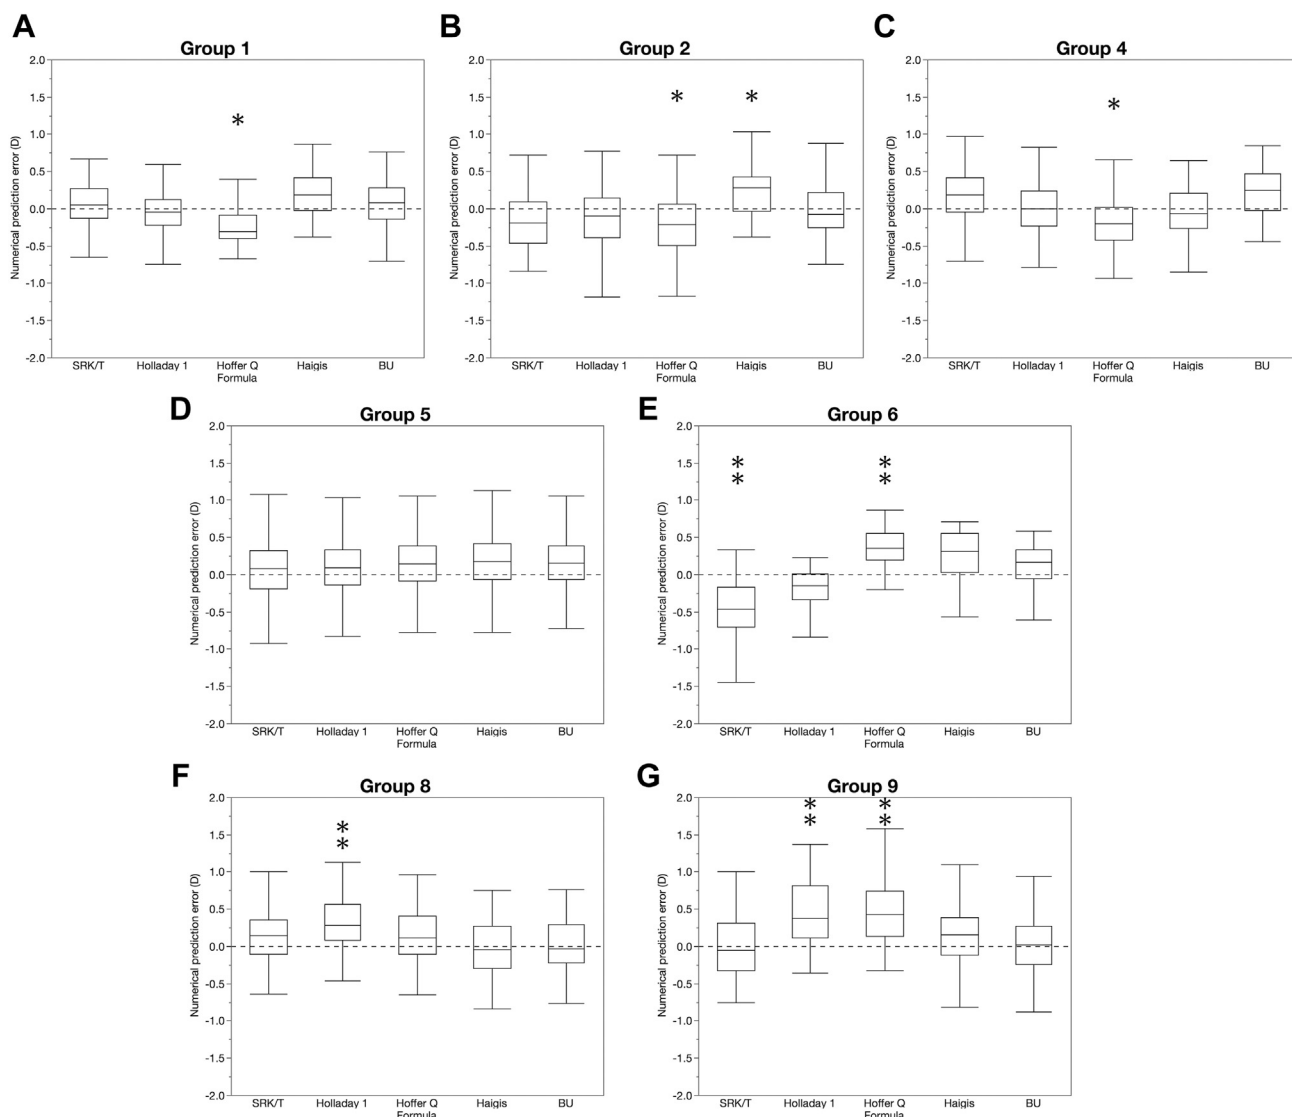


FIGURE 2. Distribution of the numerical prediction error in refraction with the 5 intraocular lens power calculation formulas for 7 subgroups. A: Group 1; B: Group 2; C: Group 4; D: Group 5; E: Group 6; F: Group 8; G: Group 9. *Significant ($P < .05$) differences were compared with other formulas. **Significant ($P < .001$) differences were compared with other formulas. AL = axial length; CR = corneal radius; AL/CR ratio = axial length-to-corneal radius ratio; BU = Barrett Universal II; D = diopters.

In eyes with normal ALs and high AL/CR ratios, the SRK/T formula had a strong tendency toward myopic results. Reitblat and colleagues⁵³ reported that the IOL power calculations for eyes with steep corneas yielded myopic prediction errors with the SRK/T formula. Melles and colleagues⁵⁴ reported that the SRK/T formula tended to overestimate the IOL power in eyes with steep corneas. The current study found that, in steep corneas with medium ALs, a high degree of myopia was predicted, whereas steep corneas with long ALs were not predicted to have as high a degree of myopia. Sheard and colleagues⁵⁵ reported a systemic error arising from the equations used to predict the corneal height when using the SRK/T formula. In eyes with normal ALs and

high AL/CR ratios, the corneas are relatively steep; therefore, the corneal height and ELP lengthened, which may cause the myopic trend with the SRK/T formula associated with normal ALs and high AL/CR ratios. Moreover, the SRK/T formula defined the AL (corrected), W (corneal diameter), and corneal height as follows⁷:

- If $AL \leq 24.2$ mm, AL (corrected) = AL
- If $AL > 24.2$ mm, the AL (corrected) = $-3.446 + 1.715 \times AL - 0.0237 \times AL^2$
- $W = -5.41 + 0.58413 \times AL \text{ (corrected)} + 0.098 \times K$
- Corneal height = $CR - \sqrt{(CR^2 - W^2/4)}$

TABLE 2. Median and Mean Absolute Errors for All Formulas and Groups

Group	AL	AL/CR	n	S (D)	Holla (D)	Hoff (D)	Ha (D)	BU (D)	P Value
1	Short	Low	29	0.20 (0.26 ± 0.26 ^a)	0.20 (0.26 ± 0.25 ^a)	0.34 (0.36 ± 0.26 ^a)	0.26 (0.38 ± 0.35 ^a)	0.19 (0.32 ± 0.31 ^a)	NS
2		Moderate	33	0.24 (0.35 ± 0.31 ^a)	0.22 (0.31 ± 0.26 ^a)	0.26 (0.34 ± 0.30 ^a)	0.34 (0.35 ± 0.25 ^a)	0.23 (0.30 ± 0.26 ^a)	NS
3		High	0	NA	NA	NA	NA	NA	NA
4	Medium	Low	84	0.25 (0.31 ± 0.24 ^a)	0.23 (0.26 ± 0.21 ^a)	0.28 (0.32 ± 0.23 ^a)	0.24 (0.29 ± 0.23 ^a)	0.30 (0.33 ± 0.24 ^a)	NS
5		Moderate	832	0.26 (0.33 ± 0.27 ^a)	0.25 (0.31 ± 0.26 ^a)	0.26 (0.33 ± 0.27 ^a)	0.27 (0.34 ± 0.29 ^a)	0.26 (0.32 ± 0.28 ^a)	NS
6		High	26	0.46 (0.50 ± 0.36 ^a)	0.21 (0.28 ± 0.26 ^a)	0.44 (0.40 ± 0.21 ^a)	0.38 (0.36 ± 0.23 ^a)	0.28 (0.26 ± 0.17 ^a)	S vs. BU and Holla ($P < .05$ for all comparisons) Hoff vs. Holla ($P < .05$)
7	Long	Low	0	NA	NA	NA	NA	NA	NA
8		Moderate	44	0.29 (0.33 ± 0.25 ^a)	0.39 (0.40 ± 0.29 ^a)	0.25 (0.32 ± 0.27 ^a)	0.27 (0.31 ± 0.26 ^a)	0.22 (0.31 ± 0.25 ^a)	NS
9		High	87	0.31 (0.35 ± 0.26 ^a)	0.40 (0.50 ± 0.38 ^a)	0.43 (0.49 ± 0.36 ^a)	0.27 (0.34 ± 0.28 ^a)	0.25 (0.31 ± 0.25 ^a)	Holla vs. S, Ha and BU ($P < .05$ for all comparisons) Hoff vs. S, Ha and BU ($P < .05$ for all comparisons)

AL = axial length; AL/CR = axial length length-to to-corneal radius ratio; BU = Barrett Universal II; D = diopters; Ha = Haigis; Hoff = Hoffer Q; Holla = Holladay 1; NA = not applicable; NS = not significant; S = SRK/T.

^aValues in parentheses indicate means ± SD.

TABLE 3. Percentage of Eyes with a Refractive Prediction Error within ± 0.50 D and ± 1.00 D

Group	AL	AL/CR	No.	S (%)	Holla (%)	Hoff (%)	Ha (%)	BU (%)	P Value
Within ±0.50 D									
1	Short	Low	29	86.2	82.8	79.3	75.9	75.9	.565 ^a
2		Moderate	33	75.8	81.8	69.7	78.8	84.8	.391 ^a
3		High	0	NA	NA	NA	NA	NA	NA
4	Medium	Low	84	78.6	84.5	81.0	83.3	79.8	.722 ^a
5		Moderate	832	78.2	81.6	79.4	78.0	80.4	.679 ^a
6		High	26	53.8	80.8	61.5	69.2	88.5	S vs BU (<i>P</i> < .05)
7	Long	Low	0	NA	NA	NA	NA	NA	NA
8		Moderate	44	79.5	61.4	77.3	84.1	84.1	Holla vs. Ha and BU (<i>P</i> < .05 for all comparisons)
9		High	87	75.9	60.9	55.2	79.3	83.9	Holla vs. Ha and BU (<i>P</i> < .05 for all comparisons) Hoff vs. S, Ha and BU (<i>P</i> < .05 for all comparisons)
Within ± 1.00 D									
1	Short	Low	29	96.6	96.6	96.6	93.1	96.6	.856
2		Moderate	33	97.0	97.0	97.0	97.0	97.0	1.000 ^a
3		High	0	NA	NA	NA	NA	NA	NA
4	Medium	Low	84	100	100	98.8	98.8	100	.406 ^a
5		Moderate	832	97.8	98.1	97.1	96.0	97.1	.841 ^a
6		High	26	92.3	96.2	100	100	100	.171 ^a
7	Long	Low	0	NA	NA	NA	NA	NA	NA
8		Moderate	44	95.5	95.5	97.7	97.7	97.7	.788 ^a
9		High	87	75.9	60.9	55.2	79.3	83.9	Holla vs. S and Ha (<i>P</i> < .05 for all comparisons) Holla vs. BU (<i>P</i> < .001) Hoff vs. BU (<i>P</i> < .05)

AL = axial length; AL/CR = axial length length-to-to-corneal radius ratio; BU = Barrett Universal II; D = diopters; Ha = Haigis; Hoff = Hoffer Q; Holla = Holladay 1; NA = not applicable; NS = not significant; S = SRK/T.

^aValues are means \pm SD.

Therefore, the longer the AL becomes, the longer the difference between the AL and the AL (corrected) for the SRK/T formula becomes. It suggests that for medium ALs and high AL/CR ratios, the AL (corrected) may be calculated as not being so short and the corneal height may not be canceled by the AL (corrected).

Calculating the IOL powers in highly myopic eyes also remains a challenge that often leads to unexpected postoperative hyperopia.^{12,26–30,56} In eyes with long ALs, both the Holladay 1 and Hoffer Q formulas exhibited a hyperopic trend. Several studies have reported the same result.^{12,27–30} Zhang and colleagues⁵⁷ reported that in eyes with long ALs (over 29 mm), the SRK/T formula had a lower MedAE than the Haigis formula. In the current study, there were no significant differences between the SRK/T and Haigis formulas in eyes with long ALs. We found that in the subgroups with medium AL/CR ratios, the Holladay 1 formula was less accurate, whereas the Hoffer Q formula was as accurate as other formulas. The following reasons may explain this. In eyes with long ALs with medium AL/CR ratios, there are great variations in the postopera-

tive ACDs with the Holladay 1 formula, whereas the postoperative ACD with the Hoffer Q formula is constant (6.5). The Holladay 1 formula uses the Pythagorean theorem to calculate the ELP, similar to the SRK formula, and it is possible that the difference in the method of calculating the postoperative ACD may cause a prediction error.

In other words, the third-generation formulas (Hoffer Q, SRK-T, and Holladay 1) are less accurate in eyes with medium and long ALs with high AL/CR ratios possibly because these formulas calculate the ELP or postoperative ACD obtained from the AL and the corneal power. In eyes with long ALs with high AL/CR ratios, the ELP for the SRK/T formula becomes longer than those for the Holladay 1 and Hoffer Q formulas, because the AL for the SRK/T formula is corrected in eyes with long ALs. Therefore, the SRK/T formula was accurate in long ALs with high AL/CR ratios.

The current study had some limitations. First, the study sample did not include eyes with short ALs with high AL/CR ratios or long ALs with low AL/CR ratios. In this study, the definitions of short and long ALs were based on a

TABLE 4. Studies Reporting AL, CR, and AL/CR

Origin Study	N	Mean \pm SD Age (y) or Age Range	AL/CR Ratio or Mean \pm SD Ratio	Mean AL or Mean \pm SD AL (mm)	Mean CR or Mean \pm SD CR (mm)
Myanmar ³⁵	1,498	56.2 \pm 11.5	2.99	22.76 \pm 1.05 ^a	7.6 \pm 0.50 ^a
Jordan ³⁴	1,093	17-40	3.00 \pm 0.13 ^a	23.13 \pm 1.00 ^a	7.7 \pm 0.30 ^a
Iran ³⁷	4,820	40-64	3.03	23.14	7.63
China ⁴⁰	3,728	69.5 \pm 8.05 ^a (29-88)	3.03 \pm 0.12 ^a	23.04 \pm 1.49 ^a	–
China ³⁹	1,717	40-84	3.04	23.23 \pm 1.17 ^a	7.6 \pm 0.27 ^a
Nigeria ³⁸	350	34.8 \pm 11.2 ^a (18-60)	3.04 \pm 0.10 ^a	23.78 \pm 0.91 ^a	7.8 \pm 0.28 ^a
Spain ³¹	583	20.32 \pm 2.82 ^a	3.05 \pm 0.14 ^a	23.61 \pm 1.05 ^a	7.7 \pm 0.25 ^a
India ³⁶	2,785	57.8 \pm 10.1 ^a (40-83)	3.08 \pm 0.13 ^a	23.45 \pm 1.10 ^a	7.61 \pm 0.26 ^a
China ⁴¹	6,099	62.56 \pm 8.00 ^a (50-96)	3.08 \pm 1.07 ^a	23.53 \pm 1.34 ^a	–
Current study	1,135	73.1 \pm 7.78 ^a (43-93)	3.15 \pm 0.19 ^a	24.00 \pm 1.53 ^a	7.6 \pm 0.25 ^a

AL = axial length; AL/CR = axial length to corneal radius ratio; CR = corneal radius; SD = standard deviation.

^aThese values are means \pm SD (if they were mentioned in the original article).

previous study,⁵⁸ and the AL/CR ratio values were divided depending on the 10th and 90th percentiles. Therefore, the number of peripheral subgroups was inevitably small. In addition, the authors believe this trend is reasonable because the AL/CR ratios tend to become high in myopic eyes and vice versa, as shown in the current study. However, despite these small numbers, significant differences were found in groups 6, 8, and 9, which are meaningful. Second, the study sample did not include short eyes (AL, <21.0 mm) or very long eyes (AL, >30.0 mm).

In conclusion, the mean AL/CR ratio in Japan was the highest compared with previously published data from other countries. The AL/CR ratio explains the total variation in the SE better than the AL alone. The SRK/T formula performed less accurately in eyes with medium ALs with high AL/CR ratios. Furthermore, the Holladay 1 and Hoffer Q formulas performed less accurately in eyes with long ALs with high AL/CR ratios. The Barrett Uni-

versal II formulas performed well across a range of ALs and AL/CR ratios. Surgeons should pay attention to the selection of IOL power calculation formulas in eyes with high AL/CR ratios.

CRedit AUTHORSHIP CONTRIBUTION STATEMENT

MIKI KAMIKAWATOKO OMOTO: CONCEPTUALIZATION, Methodology, Software, Writing - original draft. **Hidemasa Torii:** Writing - review & editing. **Ken Hayashi:** Data curation, Writing - review & editing. **Masahiko Ayaki:** Writing - review & editing. **Kazuo Tsubota:** Writing - review & editing. **Kazuno Negishi:** Conceptualization, Methodology, Writing - review & editing, Supervision.

ALL AUTHORS HAVE COMPLETED AND SUBMITTED THE ICMJE FORM FOR DISCLOSURE OF POTENTIAL CONFLICTS OF INTEREST and none were reported.

Funding/Support: No outside funding was received for this study.

Financial Disclosures: K.N. has received support from Fuji Xerox Co (Tokyo, Japan); and has received personal fees from Alcon Japan (Tokyo, Japan), Santen Pharmaceutical (Osaka, Japan), Hoya (Tokyo, Japan), Abbott Medical Optics (Santa Ana, California), Senju Pharmaceutical (Osaka, Japan), and Kowa (Nagoya, Japan); and has received personal fees from RE Medical Inc. (Osaka, Japan), BLJ (Tokyo, Japan), Wakamoto (Tokyo, Japan), Universal View (Tokyo, Japan), M3 (Tokyo, Japan), Toray Industries (Tokyo, Japan), Chuo Sangio (Hyogo, Japan), Kowa Pharmaceutical (Tokyo, Japan), Otsuka Pharmaceutical (Tokyo, Japan), Qualitas (Tokyo, Japan), NIDEK (Aichi, Japan), and Carl Zeiss Meditec (Jena, Germany); and holds patent rights for potential products for myopia suppression.

H.T. has received research support and personal fees from Fuji Xerox (Tokyo, Japan), Otsuka Pharmaceutical (Tokyo, Japan), Santen Pharmaceutical (Osaka, Japan), Hoya (Tokyo, Japan), Alcon Japan (Tokyo, Japan), MediProduce (Tokyo, Japan), Senju Pharmaceutical (Osaka, Japan), Carl Zeiss Meditec (Jena, Germany), Rohto Pharmaceutical (Osaka, Japan), and Tsubota Laboratory, Inc. (Tokyo, Japan).

K.T. has received research support and personal fees from Santen Pharmaceutical (Osaka, Japan), Otsuka Pharmaceutical (Tokyo, Japan), Jins (Tokyo, Japan), Wakasa Seikatsu (Kyoto, Japan), Wakamoto Pharmaceutical (Tokyo, Japan), Toshiba Materials (Tokyo, Japan), Asahi Glass (Tokyo, Japan), Toray (Tokyo, Japan), Plus One Marketing (Tokyo, Japan), Laboratoires Thea, AMO Japan K.K. (Tokyo, Japan), Tear Solutions (Tokyo, Japan), Novaliq, Tissue Tech, Kowa (Aichi, Japan), Rohto Pharmaceutical (Osaka, Japan), Pfizer, R-Tech Ueno (Tokyo, Japan), Ophtechs (Hyogo, Japan), Alcon Japan (Tokyo, Japan), NIDEK (Aichi, Japan), Ocular Surface Research & Education Foundation, Tsubota Laboratory (Tokyo, Japan). In addition, patents are pending or granted with Jins (Tokyo, Japan), Asahi Glass (Tokyo, Japan), and Toshiba Materials (Tokyo, Japan).

M.O., K.H., and M.A. have reported that they have no relationships relevant to the contents of this paper to disclose.

The authors thank Dr. Yasunori Sato (Keio University Hospital Clinical and Translation Research Center) for guidance and support in conducting the statistical analyses. The authors also thank Lynda Charters for English editing.

REFERENCES

- Haigis W, Lege B, Miller N, Schneider B. Comparison of immersion ultrasound biometry and partial coherence interferometry for intraocular lens calculation according to Haigis. *Graefes Arch Clin Exp Ophthalmol* 2000;238:765–773.
- Findl O, Drexler W, Menapace R, Heinzl H, Hitzinger CK, Fercher AF. Improved prediction of intraocular lens power using partial coherence interferometry. *J Cataract Refract Surg* 2001;27:861–867.
- Olsen T. Calculation of intraocular lens power: a review. *Acta Ophthalmol Scand* 2007;85:472–485.
- Norrby S. Sources of error in intraocular lens power calculation. *J Cataract Refract Surg* 2008;34:368–376.
- Sahin A, Hamrah P. Clinically relevant biometry. *Curr Opin Ophthalmol* 2012;23:47–53.
- Hoffer KJ. The Hoffer Q formula: a comparison of theoretic and regression formulas. *J Cataract Refract Surg* 1993;19:700–712.
- Retzlaff JA, Sanders DR, Kraff MC. Development of the SRK/T intraocular lens implant power calculation formula. *J Cataract Refract Surg* 1990;16:333–340.
- Holladay JT, Prager TC, Chandler TY, Musgrove KH, Lewis JW, Ruiz RS. A three-part system for refining intraocular lens power calculations. *J Cataract Refract Surg* 1988;14:17–24.
- Barrett GD. An improved universal theoretical formula for intraocular lens power prediction. *J Cataract Refract Surg* 1993;19:713–720.
- Narvaez J, Zimmerman G, Stulting RD, Chang DH. Accuracy of intraocular lens power prediction using the Hoffer Q, Holladay 1, Holladay 2, and SRK/T formulas. *J Cataract Refract Surg* 2006;32:2050–2053.
- Aristodemou P, Knox Cartwright NE, Sparrow JM, Johnston RL. Formula choice: Hoffer Q, Holladay 1, or SRK/T and refractive outcomes in 8108 eyes after cataract surgery with biometry by partial coherence interferometry. *J Cataract Refract Surg* 2011;37:63–71.
- Kane JX, Van Heerden A, Atik A, Petsoglou C. Intraocular lens power formula accuracy: Comparison of 7 formulas. *J Cataract Refract Surg* 2016;42:1490–1500.
- Ladas JG, Siddiqui AA, Devgan U, Jun AS. A 3-D "super surface" combining modern intraocular lens formulas to generate a "super formula" and maximize accuracy. *JAMA Ophthalmol* 2015;133:1431–1436.
- Clarke GP. FullMonte IOL. Available at: <https://fullmonteio.com/>. Accessed January 7, 2017.
- Hill WE. Hill-RBF method. Available at: <http://rbfcalculator.com/online/index.html>. Accessed January 7, 2017.
- Kane JX, Van Heerden A, Atik A, Petsoglou C. Accuracy of 3 new methods for intraocular lens power selection. *J Cataract Refract Surg* 2017;43:333–339.
- Katz J, Tielsch JM, Sommer A. Prevalence and risk factors for refractive errors in an adult inner city population. *Invest Ophthalmol Vis Sci* 1997;38:334–340.
- Dandona R, Dandona L, Srinivas M, et al. Refractive error in children in a rural population in India. *Invest Ophthalmol Vis Sci* 2002;43:615–622.
- Kempner JH, Mitchell P, Lee KE, et al. The prevalence of refractive errors among adults in the United States, Western Europe, and Australia. *Arch Ophthalmol* 2004;122:495–505.
- Bourne RR, Dineen BP, Ali SM, Noorul Huq DM, Johnson GJ. Prevalence of refractive error in Bangladeshi adults: results of the National Blindness and low vision survey of Bangladesh. *Ophthalmology* 2004;111:1150–1160.
- Xu L, Li J, Cui T, et al. Refractive error in urban and rural adult Chinese in Beijing. *Ophthalmology* 2005;112:1676–1683.
- Sawada A, Tomidokoro A, Araie M, Iwase A, Yamamoto T, Tajimi Study G. Refractive errors in an elderly Japanese population: the Tajimi Study. *Ophthalmology* 2008;115:363–370 e3.
- Nakamura Y, Nakamura Y, Higa A, et al. Refractive errors in an elderly rural Japanese population: the Kumejima study. *PLoS One* 2018;13:e0207180.
- Savini G, Negishi K, Hoffer KJ, Schiano Lomoriello D. Refractive outcomes of intraocular lens power calculation using different corneal power measurements with a new optical biometer. *J Cataract Refract Surg* 2018;44:701–708.
- Grosvenor T. High axial length/corneal radius ratio as a risk factor in the development of myopia. *Am J Optom Physiol Opt* 1988;65:689–696.
- He X, Zou H, Lu L, et al. Axial length/corneal radius ratio: association with refractive state and role on myopia detection combined with visual acuity in Chinese schoolchildren. *PLoS One* 2015;10:e0111766.
- Ip JM, Huynh SC, Kifley A, et al. Variation of the contribution from axial length and other oculometric parameters to refraction by age and ethnicity. *Invest Ophthalmol Vis Sci* 2007;48:4846–4853.
- Ojaimi E, Rose KA, Morgan IG, et al. Distribution of ocular biometric parameters and refraction in a population-based study of Australian children. *Invest Ophthalmol Vis Sci* 2005;46:2748–2754.
- Ip JM, Huynh SC, Robaei D, et al. Ethnic differences in the impact of parental myopia: findings from a population-based study of 12-year-old Australian children. *Invest Ophthalmol Vis Sci* 2007;48:2520–2528.
- Kimura S, Hasebe S, Miyata M, Hamasaki I, Ohtsuki H. Axial length measurement using partial coherence interferometry in myopic children: repeatability of the measurement and comparison with refractive components. *Jpn J Ophthalmol* 2007;51:105–110.
- Gonzalez Blanco F, Sanz Fernandez JC, Munoz Sanz MA. Axial length, corneal radius, and age of myopia onset. *Optom Vis Sci* 2008;85:89–96.
- Iyamu E, Iyamu J, Obiakor CI. The role of axial length-corneal radius of curvature ratio in refractive state categorization in a Nigerian population. *ISRN Ophthalmol* 2011;2011:138941.
- User Group for Laser Interference Biometry. Optimized IOL Constants for the ZEISS IOLMaster calculated from patient data on file (as of Oct 31, 2016). [Accessed 14 May 2020].
- Mallen EA, Gammoh Y, Al-Bdour M, Sayegh FN. Refractive error and ocular biometry in Jordanian adults. *Ophthalmic Physiol Opt* 2005;25:302–309.
- Warrier S, Wu HM, Newland HS, et al. Ocular biometry and determinants of refractive error in rural Myanmar: the Meiktila Eye Study. *Br J Ophthalmol* 2008;92:1591–1594.
- Pan CW, Wong TY, Chang L, et al. Ocular biometry in an urban Indian population: the Singapore Indian Eye Study (SINDI). *Invest Ophthalmol Vis Sci* 2011;52:6636–6642.

37. Hashemi H, Khabazkhoob M, Miraftab M, et al. Axial length-to-corneal radius of curvature ratio and refractive errors. *J Ophthalmic Vis Res* 2013;8:220–226.
38. Badmus SA, Ajaiyeoba AI, Adegbehingbe BO, Onakpoya OH, Adeoye AO. Axial length/corneal radius of curvature ratio and refractive status in an adult Nigerian population. *Niger J Clin Pract* 2017;20:1328–1334.
39. Wong TY, Foster PJ, Ng TP, Tielsch JM, Johnson GJ, Seah SK. Variations in ocular biometry in an adult Chinese population in Singapore: the Tanjong Pagar Survey. *Invest Ophthalmol Vis Sci* 2001;42:73–80.
40. Cao X, Hou X, Bao Y. The ocular biometry of adult cataract patients on lifeline express hospital eye-train in rural China. *J Ophthalmol* 2015;2015:171564.
41. He J, Lu L, He X, et al. The relationship between crystalline lens power and refractive error in older Chinese adults: the Shanghai Eye Study. *PLoS One* 2017;12:e0170030.
42. Foo VH, Verkicharla PK, Ikram MK, et al. Axial length/corneal radius of curvature ratio and myopia in 3-year-old children. *Transl Vis Sci Technol* 2016;5:5.
43. Scheiman M, Gwiazda J, Zhang Q, et al. Longitudinal changes in corneal curvature and its relationship to axial length in the Correction of Myopia Evaluation Trial (COMET) cohort. *J Optom* 2016;9:13–21.
44. He M, Xiang F, Zeng Y, et al. Effect of time spent outdoors at school on the development of myopia among children in China: a randomized clinical trial. *JAMA* 2015;314:1142–1148.
45. Grosvenor T, Scott R. Role of the axial length/corneal radius ratio in determining the refractive state of the eye. *Optom Vis Sci* 1994;71:573–579.
46. He J, Xu X, Zhu J, et al. Lens power, axial length-to-corneal radius ratio, and association with diabetic retinopathy in the adult population with type 2 diabetes. *Ophthalmology* 2017;124:326–335.
47. Morgan IG, Ohno-Matsui K, Saw SM. Myopia. *Lancet* 2012;379(9827):1739–1748.
48. Yotsukura E, Torii H, Inokuchi M, et al. Current prevalence of myopia and association of myopia with environmental factors among schoolchildren in Japan. *JAMA Ophthalmol* 2019;137:1233–1239.
49. Fink AM, Gore C, Rosen ES. Refractive lensectomy for hyperopia. *Ophthalmology* 2000;107:1540–1548.
50. Holladay JT, Gills JP, Leidlein J, Cherchio M. Achieving emmetropia in extremely short eyes with two piggyback posterior chamber intraocular lenses. *Ophthalmology* 1996;103:1118–1123.
51. Gokce SE, Zeiter JH, Weikert MP, Koch DD, Hill W, Wang L. Intraocular lens power calculations in short eyes using 7 formulas. *J Cataract Refract Surg* 2017;43:892–897.
52. Shrivastava AK, Behera P, Kumar B, Nanda S. Precision of intraocular lens power prediction in eyes shorter than 22 mm: an analysis of 6 formulas. *J Cataract Refract Surg* 2018;44:1317–1320.
53. Reitblat O, Levy A, Kleinmann G, Lerman TT, Assia EI. Intraocular lens power calculation for eyes with high and low average keratometry readings: comparison between various formulas. *J Cataract Refract Surg* 2017;43:1149–1156.
54. Melles RB, Holladay JT, Chang WJ. Accuracy of intraocular lens calculation formulas. *Ophthalmology* 2018;125:169–178.
55. Sheard RM, Smith GT, Cooke DL. Improving the prediction accuracy of the SRK/T formula: the T2 formula. *J Cataract Refract Surg* 2010;36:1829–1834.
56. Omoto MK, Torii H, Masui S, Ayaki M, Tsubota K, Negishi K. Ocular biometry and refractive outcomes using two swept-source optical coherence tomography-based biometers with segmental or equivalent refractive indices. *Sci Rep* 2019;9:6557.
57. Zhang Z, Miao Y, Fang X, Luo Q, Wang Y. Accuracy of the Haigis and SRK/T formulas in eyes longer than 29.0 mm and the influence of central corneal keratometry reading. *Curr Eye Res* 2018;43:1316–1321.
58. Hoffer KJ. Clinical results using the Holladay 2 intraocular lens power formula. *J Cataract Refract Surg* 2000;26:1233–1237.